




Controlling the
Incubation Process
Efficiently and Reliably

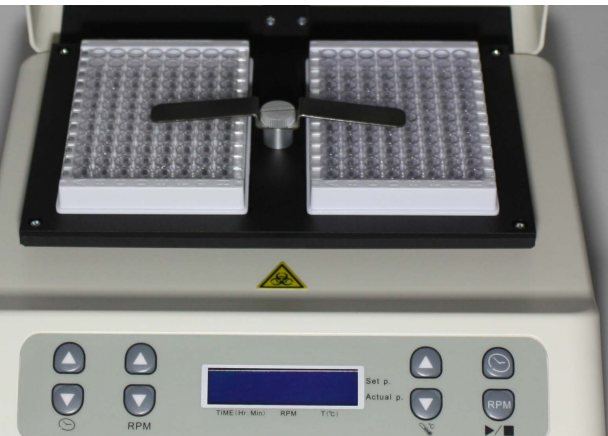


AMP Platos IS 2

Microplate Incubator and Shaker

AMP Platos IS 2 is designed for convenient and efficient incubation and mixing of microplate-based ELISA tests or cell culture plates. Two plates can be treated in parallel.

Temperature, shaker speed and time can be easily adjusted with foil buttons. Timer and shaker can be started and stopped separately. Defined settings and actual values are presented on the two-line display.

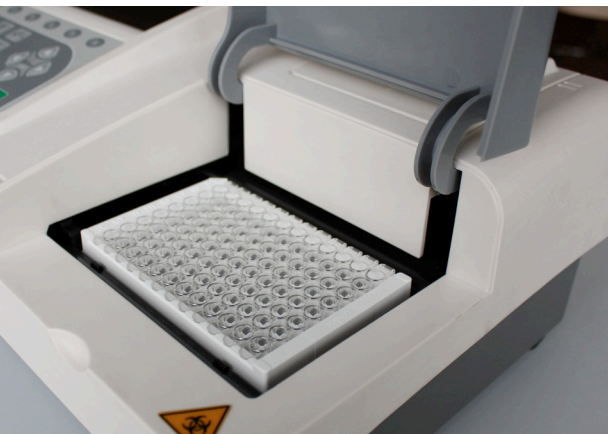

Technical Specifications

| | |
|-------------------------|--------------------------------|
| Capacity: | 2 standard microplates |
| Temperature range: | 25.0 to 60.0°C |
| Temperature setting: | In steps of 0.1°C resp. 1.0°C |
| Temperature accuracy: | ± 0.5°C |
| Temperature uniformity: | ± 0.3°C |
| Shaker speed: | 250 to 1.200 rpm |
| Speed setting: | In steps of 10 resp. 100 rpm |
| Shaker amplitude: | 2 mm |
| Timer: | 0 to 99 hours 59 minutes |
| Timer setting: | In steps of 1 resp. 10 minutes |
| Display: | 2-line LCD screen |
| Operation: | 8 foil keys |
| Power supply: | 110 - 220 VAC, 50/60 Hz |
| Power consumption: | Max. 60 W |
| Dimensions: | W 268 x D 275 x H 132 mm |
| Weight: | 6.30 kg |

AMEDA Labordiagnostik GmbH

Krenngasse 12

8010 Graz, Austria

Phone +43 316 69 80 69

Fax +43 316 69 80 69 12

E-mail office.graz@amp-med.com

www.amp-diagnostics.com



AMP Polska sp. z o.o.
AMP Diagnostics s.r.l.

Bolesława Prusa 37/1, 30-117 Kraków, Poland, Phone: +48 12 294 02 78, E-mail: office.krakow@amp-med.com
Str. Fabricii 118-A, 400632 Cluj-Napoca, Romania, Phone: +40 264 425 934, E-mail: office.cluj@amp-med.com